

Effect of Cardiopulmonary Bypass Machine on the Platelet Function Testing

Khalid A AlSaleh¹, Rashed B AlBakr¹, Turki B AlBacker², Rakan Al Nazer², Abdulkareem Almomen¹, Osama T Khoja³ and Tarek M Owaidah^{4*}

¹Department of Medicine, College of Medicine, King Saud University, Riyadh, Kingdom of Saudi Arabia

²Department of Cardiac Sciences, College of Medicine, King Saud University, Riyadh, Saudi Arabia

³Department of Pathology, College of Medicine, King Saud University, Riyadh, Saudi Arabia

⁴Department of Hematology and Transfusion, Alfaisal University, King Faisal Specialist Hospital, Riyadh, Saudi Arabia

*Corresponding author: Tarek M Owaidah, Professor of Hematology and Transfusion Medicine, Alfaisal University, King Faisal Specialist Hospital, Centre of excellence in thrombosis and Hemostasis, Riyadh 11533, Saudi Arabia, Tel: +966 50 531 2925, E-mail: towaidah@gmail.com

Received Date: June 07, 2021 Accepted Date: July 07, 2021 Published Date: July 09, 2021

Citation: Khalid A AlSaleh (2021) Effect of Cardiopulmonary Bypass Machine on the Platelet Function Testing. J Cardio Vasc Med 7: 1-10.

Abstract

Background: Bleeding during coronary artery bypass surgery is a leading cause of mortality. Several factors have been associated with bleeding, platelet dysfunction being the most significant.

Objective: to assess the effect of cardiopulmonary bypass machine (CPB) during cardiac surgery on platelet function using Platelet Function Analyzers (PFA-100), and Multiplate Electrode Aggregometry (MEA), and correlating that with a drop in Hemoglobin (Hb).

Methods: Whole blood samples were collected preoperative and sixty minutes intraoperatively of different cardiac procedures utilizing (CPB) and tested for platelet function by PFA-100 and MEA. Complete blood count was measured using an automated hematology analyzer.

Results: A significant difference was found between pre- and intraoperative ADP and EPI measurement in PFA-100, where preoperative PFA-ADP values displayed the ability to predict the intra-op drop in Hb (P -value 0.01, correlation coefficient 0.4699). At the same time, pre-op MEA- Ristocetin and TRAP showed an inverse correlation with an intra-op drop in Hb (-0.31 and -0.36).

Conclusion: The current study reported significant changes in platelet dysfunction in cardiac surgeries with CPB, measured by two modalities PFA-100, and MEA. While PFA-100 and MEA both detected the changes in platelet dysfunction due to CPB, PFA-100 results were sensitive and positively predicted intra-op Hb drop as compared to MEA. There was a significant

change in Hb one hour into the CPB, indicating that platelet transfusion might help decrease Intra- and postoperative bleeding independent of the platelet count as they are dysfunctional. PFA-100 results can be relied upon for distinction of high-risk cardiac surgery patients for bleeding and can be used for clinical decision making to improve patient outcome.

Keywords: Cardio-Pulmonary Bypass Machine; PFA-100; Platelet Dysfunction; Multiplate Electrode Aggregometry

Abbreviation: Adenosine diphosphate (ADP); Aspirin (ASA); Epinephrine (EPI); Cardiopulmonary Bypass (CPB); Coronary Artery Bypass Graft (CABG); Platelet Function Analyzer (PFA); Multiplate Electrode Aggregometry (MEA)

Introduction

Conflicting reports exist in the literature concerning the role of Platelet function analyzer (PFA-100) in identifying high-risk patients for bleeding during CPB [1]; ranging from high negative to high positive predictive values in cardiac surgery patients for postoperative transfusion management [2]. Multiple factors play a role related to bleeding during CPB, which could be due to the operative procedure or the operator and type of procedure. Platelet dysfunction as an entity by itself could be one of the causes of hemorrhage. A worldwide survey of 37 countries and 202 laboratories reported that PFA and Multiplate Electrode aggregometry (MEA) are used for screening of platelet function disorders in 53% and 12% of laboratories, respectively [3]. This extensive use, in turn, leads to clinical decisions which determine patient outcome. PFA-100 is used more excessively than MEA for the screening of primary hemostatic disorders; however, a meta-analysis showed that the majority of studies reporting diagnostic accuracy and sensitivity of PFA-100 lacked quality and reporting requirements, impeding precise characterization of its clinical utility [1]. Thus, emphasizing the need for evidence-based critical evaluation of the diagnostic performance of PFA-100 and MEA for platelet dysfunction in the clinical setting.

The routine procedure of CPB still requires immediate therapeutic improvements and optimization strategies to deal with pre- and intraoperative complications, such as functional haemostatic defects leading to its hall-mark of bleeding [4]. Bleeding incidence after CPB varies from 5–25%, and platelet dysfunction is possibly the most plausible yet controversial explanation for coagulopathy related to CPB [5]. Quantitative, as well as qualitative aspects of platelet dysfunction, participate in thromboembolism and microvascular injury [6]. However, in CPB related hemostatic defects, functional abnormalities of platelets are extrinsic rather than intrinsic. This is depicted by optimal platelet reactivity in CPB in-vitro and a minimum amount of degranulated circulating platelets [7].

Owing to the paramount importance of platelet function in bleeding diathesis with its subsequent influence on therapeutic strategies and patient outcome, there is a dire need to address two major aspects of cardiac surgery. Firstly, the different modalities of cardiac surgery utilizing CPB and its effect on platelet function; and secondly the evaluation of the diagnostic performance of point-of-care testing devices dedicated to the measurement of platelet function, such as PFA-100, MEA, and VerifyNow System [2, 8-11].

The current study planned to evaluate two methods PFA-100 & MEA side by side comparing and identifying which one is more sensitive in predicting the risk of intra-op bleeds. We presumed that the use of sensitive, time saving and efficient test for prediction of high-risk patients would govern accurate clinical decisions, leading to better patient outcome and reduced mortality associated with CPB.

Methods

Patient selection

The study was approved by the Institutional Review Board of College of Medicine, King Saud University, Kingdom of Saudi Arabia. Samples were collected after informed consent indicating the purpose of the study and the right of the participant to withdraw at any time without any obligation towards the study team. Blood samples from ($n=34$) adult patients were recruited from KKUH, having routine normal coagulation tests prior to the different cardiac procedures, including valve replacement, coronary artery bypass etc. were collected at two points in time; at the beginning of the CPB and 60 mins into CPB. All patients going for CPB procedure were advised to stop antiplatelet therapy five days prior to the procedure.

Before starting the CPB for every patient, 20cc blood from central-line access point was collected for complete blood count (CBC), and platelet function tests. The second time-point

was 60 min after the start of CPB. The two blood samples at each point in time were collected as one sample in the EDTA tube for CBC, and in the Lithium tube for platelet function tests. Citrated blood in sodium citrate tubes was aspirated. Platelet and blood products were transfused as needed as per the discretion of the cardiac surgeon.

Platelet function testing

PFA-100 analyzer and MEA were used to measure the extent of platelet dysfunction pre- and intra- CPB. Complete blood counts including HCT, Hb and PLT counts were measured using a hematology analyzer (Advia 120; Bayer, Tarrytown, NY, USA), and platelet function analysis by PFA-100 (Siemens Healthcare Diagnostics, Malvern, PA, USA). Disposable cartridges on high shear rates were used for PFA-100, containing aperture inside a membrane coated with cADP or cEPI, which induced platelet activation leading to adhesion and aggregation, resulting in occlusion of aperture. The time needed to occlude aperture and stop the blood flow is called Closure Time (CT). The longer is the closure time; the more platelet dysfunction is expected [12].

Whole blood samples from these patients were also tested by a Multiplate analyzer (Dynabyte, Munich, Germany). Aggregation and adhesion of platelets on electrode surfaces are converted to electrical impedance which is measured by Multiplate analyzer. The test cuvette contained platelet agonists; aspirin (ASP: 15 mM), (TRAP: 1 mM), collagen (COL) (100 lg/mL), arachidonic acid (ADP 0.2 mM), and ristocetin (RISTO: 10 mg/mL). Platelet adhesion after activation results in aggregation on metal sensor causing electrical impedance between electrode wires, which was measured continuously for six minutes and analyzed after conversion to arbitrary units.

We calculated the most important parameter, which is the area under the aggregation curve (AUC). It is affected by the total height of the aggregation curve as well as by its slope and is best suited to express the overall platelet activity, and expressed as AUC*min [10]. Lower value indicates more platelet dysfunction

Definitions

Thrombin receptor-activating peptide (TRAP-6); a potent platelet activator and stimulates platelet aggregation via stimulation of platelet thrombin receptors. Aspirin or Clopidogrel cannot block this action. This means TRAP allows GpIIb/IIIa antagonists to be detected even in samples containing Aspirin (ASP) or Clopidogrel. Adenosine diphosphate (ADP) stimu-

lates platelet activation by the ADP receptors. In COL test, Collagen activates the collagen receptor, which in turn activates the platelets via arachidonic acid production. Ristocetin (RISTO) platelet aggregation test is based on the binding of RISTO-vWF (von Willebrand factor) complexes leading to the aggregation of platelets as well as their activation. Aspirin[®] inhibits this activation. This explains the ASP sensitivity of RISTO test.

Data Analysis

Descriptive statistics were computed as a baseline means, standard deviations (SD) and minimum and maximum values for continuous variables. Preoperative variables were compared to intra-operative variables for PFA-100 and MEA. We used skewness-kurtosis normality tests to find variables with non-normal distribution. Student t-test compared significance in mean values of normally distributed variables, while the Wilcoxon t-test compared significance in mean values of non-normally distributed variables. We used the software STATA v.13.0 (Stata Corp., College Station, TX, USA) in our analysis. A statistical significance threshold of $P < 0.05$ was adopted.

Results

Our study compared the effect of CPB on platelet function by using pre- and intra-operative platelet function parameters for 34 patients using PFA-100 analyzer and MEA. Data for two patients were removed due to erroneous PFA-100 values leading to 32 patients' data used for this study. Although all patients going for CPB procedure were advised to stop antiplatelet therapy five days prior to the procedure, we found 7 patients presenting with high PFA-100, suggesting some residual effect of antiplatelet.

Out of 32 patients, 9 (28.1%) were females with a mean age of 53.1 ± 15.4 (m: 52, r: 30–73 years), and 23 (71.9%) were male with a mean age of 58.9 ± 8.75 (m: 59, r: 40–79 years), where 'm' denotes the median, and 'r' denotes range.

We presumed that pre- and intra-operative measurements should show significant change towards worsening of platelet function. Pre- and intraoperative PFA-100, MEA and CBC measurements are summarized in Table-1. The variables showing greatest pre- and intraoperative variability are depicted as a Box Whisker plot in Figure-1, where one set depicts both PFA-ADP and epinephrine (EPI), and other shows only MEA-ADP and RISTO. The ADP observations for pre- and intraoperative are 32 and 31 respectively, with an increase in mean values from 125.9 ± 69.9 (m: 102, r: 54–300 sec) to 205 ± 74.9 (m: 162, r: 79–300 secs).

The EPI measurements also showed an increase in mean values from 166.8 ±72.5 (m: 187, r: 64–300 secs) to 214.2 ±42.7 (m: 210, r: 115–300 secs). This increase clearly shows worsening of platelet function. The significance of platelet function change is estimated using student t-test, both ADP and EPI show significant difference *P*-values <0.001 and 0.002, respectively.

Table-1 also summarizes MEA measurements. Overall, the tests show a decline in the measurements consistent with a decline in the aggregation [13]. A significant decline (*P*-value <0.001) in mean and median values of ADP (AUC) is observed from 81.5 ±28.3 (m: 75.5, r: 26–124 AUC*min) to 56.8 ±27.4 (m: 53.5, r: 7–39 AUC*min; a 30% decrease). A decline in ASP was

Table 1: Correlation between pre- and intra-operative PFA-100, MEA, and CBC measurements, including: mean values, standard deviation, median (m), and range (r) values

Variables	Pre-op	Intra-op	<i>P</i> -value
PFA-100			
ADP ¹	(m: 102, r: 54–300) ±69.9 125.9	(m: 162, r:79–300) ±74.9 205.0	<0.001
EPI ²	(m: 187, r: 64–300) 166.8+72.5	(m: 210, r:115–300)±42.7 214.2	0.002
Multiplate aggregation			
ADP	(m: 75.5, r: 26–124) 81.5+28.3	(m: 53.5, r: 7–39) ±27.4 56.8	<0.001
ASP ³	(m: 56.5, r: 23–122) 59.2+27.6	(m: 48.5, r: 10–112) ±30.8 50.2	0.085
COL ⁴	(m: 43.5, r: 27-97) ±19.0 50.0	(m: 35, r: 4–80) ±18.1 37.1	0.002
RISTO ⁵	(m: 72.5, r: 33–156) ±30.9 76.8	(m: 41, r: 4–181) ±37.9 50.9	0.0005
TRAP ⁶	(m: 112, r: 51–178) ±26.3 114.0	(m: 95, r: 13–179) ±36.0 100.0	0.02
CBC			
Hb ⁷	(m: 11.6, r: 71–157) ±12.5 13.7	(m: 8.3, r: 9–108) ±1.24 8.43	<0.001
HCT ⁸	(m: 34.2, r: 23.4–46.7) ±5.5 34.5	(m: 24.5, r:20.6–29.7) 25.0+2.6	<0.001
PLT ⁹	(m: 255, r: 136-884) ±131.9 264	(m:164, r: 21–724) ±112.6 185.3	<0.001
MPV ¹⁰	(m: 9.5, r:7.3–12.6) ±1.2 9.4	(m: 9.3, r: 4.2–12.7) ±1.4 9.2	0.16

1-Adenosine diphosphate (ADP). 2-Epinephrine (EPI). 3-Aspirin (ASA). 4-Collagen (COL).
 5- Ristocetin (RISTO). 6- Thrombin receptor-activating peptide (TRAP). 7-Hemoglobin (Hb). 8-Hematocrit (HCT). 9-Platelet count (PLT). 10-Mean Platelet Volume (MPV)

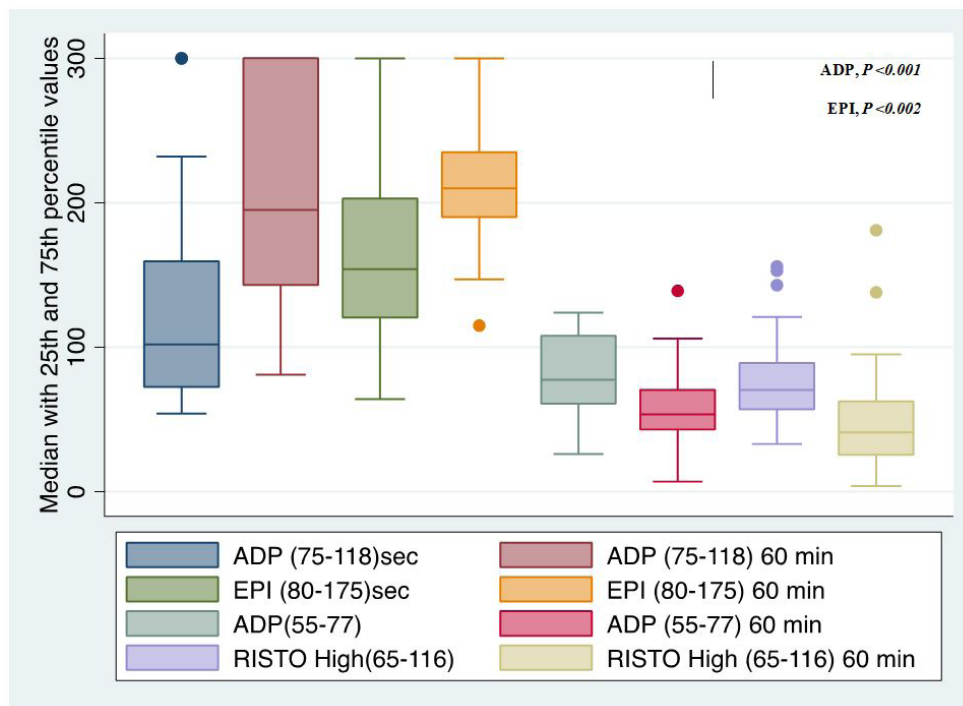


Figure 1: Box Whisker plot: on the left shows high variability of both PFA-ADP and EPI, and on the right shows only MEA-ADP and RISTO with high variability

insignificant (P -value 0.085) in mean and median values from 59.2 ± 27.6 (m: 56.5, r: 23–122 AUC*min) to 50.2 ± 30.8 (m: 48.5, r: 10–112 AUC*min; a 14% decrease). A decrease in COL was significant (P -value 0.002) in mean and median values from 50 ± 19 (m: 43.5, r: 27–97 AUC*min) to 37.1 ± 18.1 (m: 35; r: 4–80 AUC*min; a 24.5% decrease). Similarly, a significant decline was observed in RISTO and TRAP mean and median values (P -value 0.0005 and 0.02, respectively). RISTO decreased from 76.8 ± 30.9 (m: 72.5, r: 33–156 AUC*min) to 50.9 ± 37.9 (m: 41, r: 4–181 AUC*min; a 33.7% decrease). TRAP declined from 114 ± 26.3 (m: 112, r: 51–178 AUC*min) to 100 ± 36 (m: 95, r: 13–179 AUC*min, a 3.5% decrease). This little change in TRAP indicates that the sample is not contaminated with antiplatelets [10].

A significant drop in Hb values was also observed one hour after the start of CPB (P -value <0.001) from 13.7 ± 12.5 (m: 11.6, r: 71–15.7 g/L) to 8.43 ± 1.24 (m: 8.3, r: 9–10.8 g/L, a 26% decrease); HCT (P -value <0.001) from 34.5 ± 5.5 (m: 34.2, r: 23.4–46.7) to 25 ± 2.6 (m: 24.5, r: 20.6–29.7; a 27.5% decrease); PLT (P -value <0.001) from 264 ± 131.9 (m: 255) to 185.3 ± 112.6 (m: 164).

Next, we tried to answer if PFA-100 pre-op values related to intra-op drop in Hb value, as in, do we expect lower Hb

count for elevated PFA-100 values. We assumed two approaches to find the answer: first, we look for a correlation between PFA-100 variables and intra-op Hb; secondly, we run a statistical t-test which shows a significant change in Hb groups based on a dichotomy of PFA-100 variables. The binary variable was labelled 'abnormal' when both ADP and EPI values exceeded the normal range and labelled 'normal' otherwise.

We used Pearson's correlation and found a weak correlation coefficient between PFA-ADP and intra-op drop in Hb (0.4699), which is illustrated as a scatter plot in Figure-2. On the other hand, pre-op EPI showed no correlation (0.21) with the drop in intra-op Hb values, as illustrated in Figure-3. For t-test, we created a binary variable based on the values of PFA-ADP and EPI. Next, we partitioned the post-op drop in Hb based on this binary variable and compared their means using t-test. The number of patients in the abnormal set was 6, and 26 in the normal set. The difference of mean turned out to be significant (P -value 0.01), and Hb mean values for abnormal set 75 ± 0.5 (m: 75, r: 69–82) were lower than that of the normal set 86 ± 1.02 (m: 87, r: 71–108). An observation worth mentioning is that for MEA test, only pre-op RISTO and TRAP showed a weak inverse correlation with the intra-op drop in Hb (-0.31 and -0.36), while rest of the MEA variables didn't.

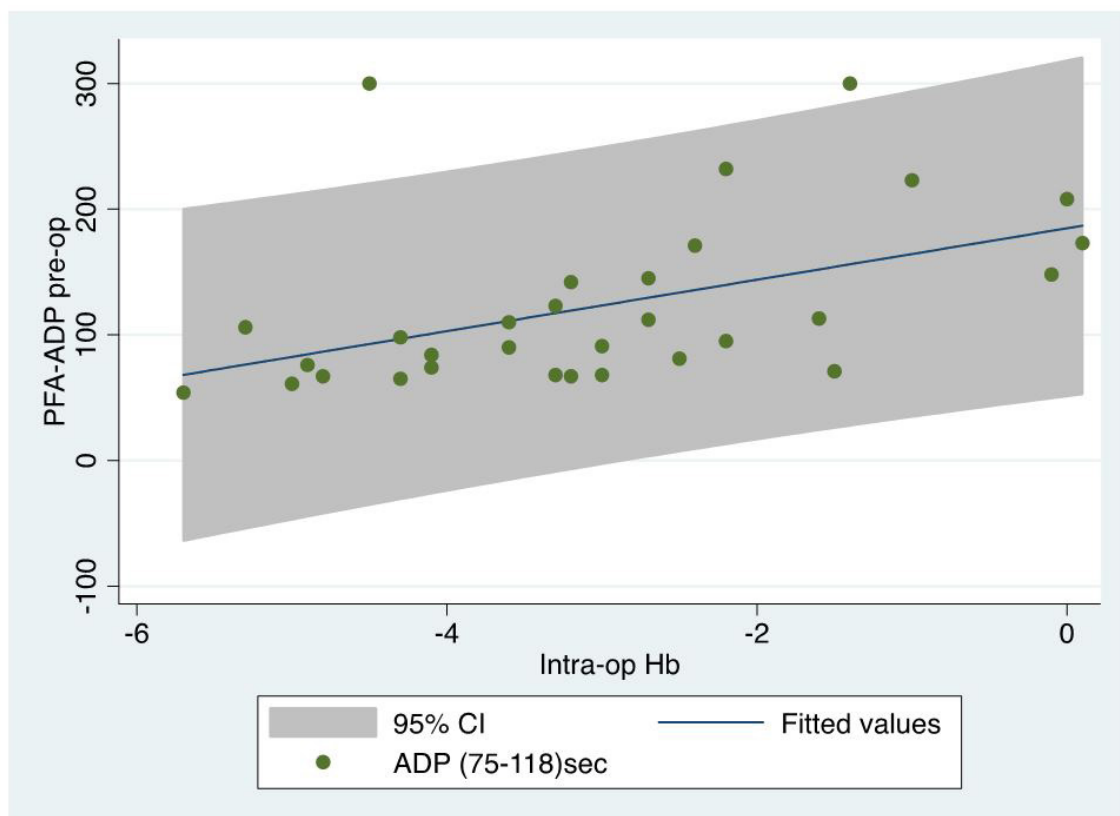


Figure 2: Scatter plot between pre-op PFA-100 ADP and intra-op drop in Hb values

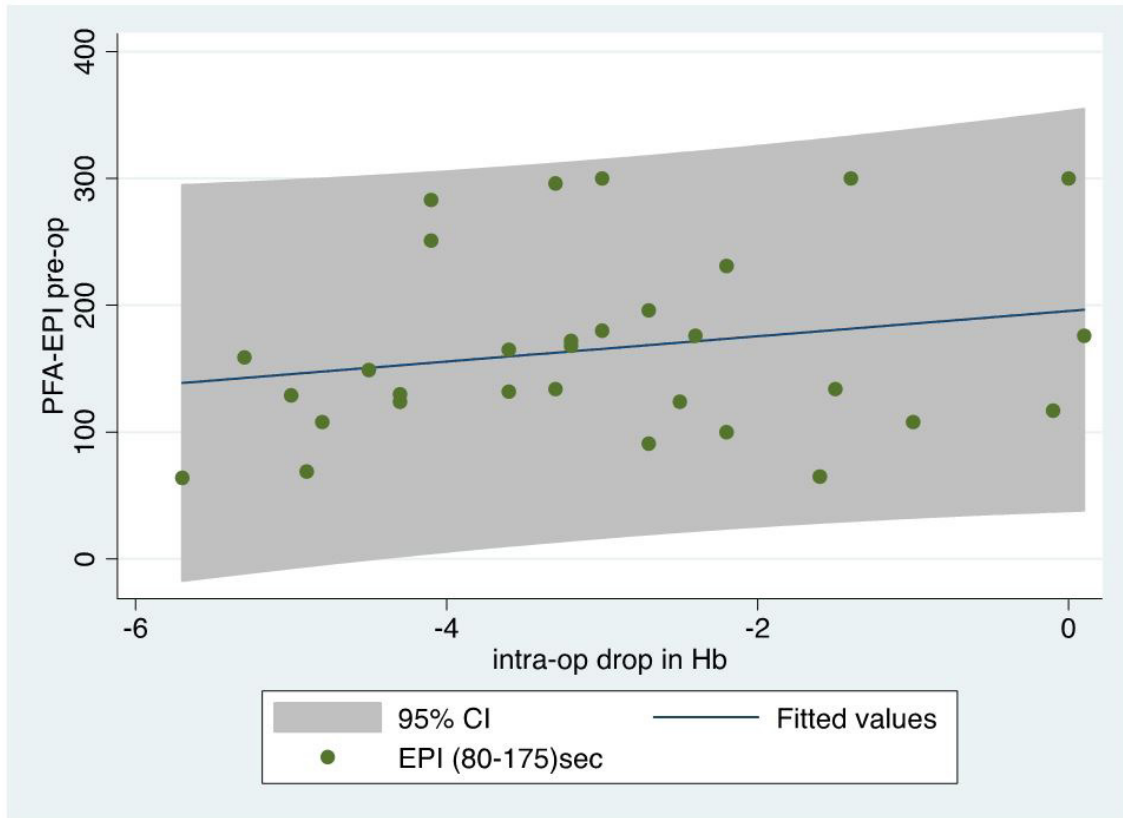


Figure 3: Scatter plot between pre-op PFA-100 EPI and intra-op drop in Hb values.

Another perspective was to look at the change in intra-op PFA-100 and MEA values against a drop in intra-op Hb. Change in intra-op PFA-100 and MEA values were obtained by subtracting intra-op from pre-op values. Similarly, the drop in intra-op Hb value was obtained by subtracting intra-op Hb from pre-op Hb. For PFA-100, change in intra-op ADP was weakly correlated to the drop in intra-op Hb (0.46). For MEA, intra-op change in ASP was weakly correlated to the drop in intra-op Hb (0.41).

Considering the gender, mean Hb levels in female patients 75 ± 0.5 (m: 73, r: 69–84g/L) were significantly lower (a 16% decrease, P -value 0.0009) than the male patients 87 ± 1.0 (m: 87, r: 71–108g/L). The same pattern was observed in HCT levels.

Discussion

Bleeding during cardiac surgery procedures makes allogeneic blood transfusion an essential requirement to maintain hemostatic blood components [9]; therefore, accurate and timely assessment of patients in need of transfusion is crucial. To meet these requirements, evaluation of platelet function along with

platelet count intra-operatively is pivotal. PFA-100 and MEA are two commonly used modalities to monitor platelet function and assess the need for transfusion and blood flow cessation [14]. Intraoperative transfusions play a crucial role in the patient outcome; therefore, sensitive and efficient platelet function test should be performed for predicting high-risk patients. The current study compared the predictive value and sensitivity of PF-100 and MEA for the identification of high-risk intra-operative patients using the intra-operative drop in Hb as a reference outcome.

The PFA-100[®] works on the principle of shear stress during vascular injury and provides quantitative data related to high shear force-associated platelet dysfunction with whole blood, and provides accurate and quantitative in-vitro measurements [14,15]. In the current study, a significant difference ($P < 0.05$) in platelet function was observed pre- and intra-CPB through PFA-ADP (125.9 ± 69.9 vs 205 ± 74.9), as well as EPI measurements (166.8 ± 72.5 vs 214.2 ± 42.7) with an increase in platelet dysfunction after starting CPB. However, conflicting results have been reported previously regarding intra-operative bleeding and its association with platelet dysfunction assessed by PFA-100 [16]. In agreement with our findings, a positive relationship between the extent of bleeding and platelet dysfunction

was reported by Ostrowsky *et al.* [17] and Raman *et al.* [18]. On the other hand, and contrary to our findings, Fattorutto *et al.* [18] and Forestier *et al.* [20] proved that PFA-100 results couldn't distinguish patients at low risk of bleeding from patients who had significant bleeding; excluding the high-risk CPB patients. In cardiothoracic procedures involving CPB, specificity and sensitivity of PFA-100 were 94% and 85%, respectively, in identifying response to platelet transfusion. Our PFA-100 results clearly predicted the outcome based on preoperative analyses as measured by correlation with intra-op drop in Hb values via Pearson correlation. Beside the Pearson co-relation test, we used a different yet meaningful approach to distinguish high and low-risk patients by generating binary variables based on values of PFA-100 ADP and EPI. The binary variable is considered abnormal when both ADP and EPI values were out of normal range. This approach is useful as some of the platelet inhibitors such as aspirin and Clopidogrel affect EPI during the test. In such a scenario, there was a significant difference between Hb levels of abnormal and normal groups.

MEA is another frequently used modality for platelet function analysis, which can be opted for the near patient setting to get prompt results. MEA has certain advantages over PFA-100, including measurement of platelet function in whole blood in the presence of other blood cells for timely assessment [21]. Although, in conformity with PFA-100 results, significant changes in platelet function were observed through MEA in pre- and intra-CPB, as indicated by a decreased aggregation depicted through less area under the curve. Meyer *et al.* showed the significance of MEA performed at the start of a surgical procedure to improve the management of blood product transfusion [22]. A positive correlation between the preoperative values of ADP from MEA and total blood transfusion during surgical intervention was reported in the study of Mengistu *et al.* [23]. However, in the current study, we found the diagnostic performance of MEA as comparatively weaker than that of PFA-100, taking an intra-op drop in Hb as an outcome. The role of MEA in lowering the number of transfusions has not been justified previously in the literature. Apropos, in the current study, MEA couldn't provide such benefits due to lower sensitivity as compared to PFA-100. Contrary to the previous studies [3], we found that PFA-100 is sensitive to detect the changes in platelet dysfunction and can be relied upon to distinguish high-risk patients for bleeding. PFA-100 also showed high variability pre- and intra-CPB in ADP and EPI; while in MEA, only ADP and RISTO show greater variability intra CPB as compared to pre-CPB values; depicting the higher sensitivity level of PFA-100.

The novelty of the current study lies in the fact that intra-operative transfusion management has been studied considering the intra-op drop in Hb as a primary outcome, which is easy to measure on-site as compared to calculations based on units transfused post cardiac surgery. Limitations of the current study lie in the fact that MEA and PFA-100 results have not been compared with the gold standard platelet function test: Light transmission aggregation [3].

This study does have a limitation of correlating the bleeding to drop in the Hb after 60 minutes of the procedure, which might reflect fluid priming the CPB or retrograde priming. Still, the timing of this measurement might be of value to limit the variability and complexity of different procedures, affect surgeons' preferences and allow the analysis of platelet dysfunction in a broader range of cardiac procedures.

Conclusion

The current study reported significant worsening in the platelet function 60 mins intra-operatively during CPB, measured by two modalities PFA-100 and MEA, which might be reversed by platelet transfusion during surgery. We found PFA-100 to be more sensitive and predictive of intra-op drop in Hb as compared to MEA,

Declarations

Authors' Contribution

KS & TO designed & developed the study. Both authors were responsible for contents & authenticity. RB, TB, RN, OK oversaw data collection, data entry, final review of data and analysis, were responsible for the direction of the study team, and facilitation of the project plan.

Funding and Source of Support

Deanship of Scientific Research, King Saud University, Researcher Supporting Project Number RSP-2019/88 for Dr. Khalid AlSaleh.

Ethics approval and consent to participate

The study was approved by the Institutional Review Board of College of Medicine, King Saud University, Kingdom of Saudi Arabia.

Consent for publication

All authors consent for publication.

Availability of data and materials

Furnished upon request.

Acknowledgement

Nazia Sadaf, MD, for her contribution in medical writing.

References

1. Karger R, Donner-Banzhoff N, Müller H-H, Kretschmer V, Hunink M (2007) Diagnostic performance of the platelet function analyzer (PFA-100®) for the detection of disorders of primary haemostasis in patients with a bleeding history—a systematic review and meta-analysis. *Platelets* 18: 249-60.
2. Paniccia R, Priora R, Liotta AA, Abbate R (2015) Platelet function tests: a comparative review. *Vascular health and risk management* 11: 133.
3. Moenen FC, Vries MJ, Nelemans PJ, van Rooy KJ, Vrancken JR, et al. (2019) Screening for platelet function disorders with Multiplate and platelet function analyzer. *Platelets* 30: 81-7.
4. Höfer J, Fries D, Solomon C, Velik-Salchner C, Ausserer J (2016) A snapshot of coagulopathy after cardiopulmonary bypass. *Clinical and Applied Thrombosis/Hemostasis* 22: 505-11.
5. Varghese S, Unni M, Mukundan N, Rai R (2005) Platelet functions in cardiopulmonary bypass surgery. *Medical Journal Armed Forces India* 61: 316-21.
6. Weerasinghe A, Taylor KM (1998) The platelet in cardiopulmonary bypass. *The Annals of thoracic surgery* 66: 2145-52.
7. Kestin AS, Valeri C, Khuri S, Loscalzo J, Ellis P, et al. (1993) The platelet function defect of cardiopulmonary bypass 1993.
8. Albanyan A, Al-Musa A, AlNounou R, Al Zahrani H, Nasr R, et al. (2015) Diagnosis of Glanzmann thrombasthenia by whole blood impedance analyzer (MEA) vs. light transmission aggregometry. *International journal of laboratory hematology* 37: 503-8.
9. Angiolillo D, Levy J, Schneider D, Jennings L (2020) The Role of Platelet Function Testing in Improving Clinical Outcomes. *The Medical Roundtable Cardiovascular Edition*.
10. Calatzis A, Loreth R, Spannagl M (2007) Multiplate® platelet function analysis-application and interpretation. V2 0/072007 Dynabyte Medical, Monachium.
11. Gibbs N (2009) Point-of-care assessment of antiplatelet agents in the perioperative period: a review. *Anaesthesia and intensive care* 37: 354-69.
12. Bogdanic D, Karanovic N, Mratinovic-Mikulandra J, Paukovic-Sekulic B, Brnic D, et al. (2017) The Role of Platelet Function Analyzer Testing in Cardiac Surgery Transfusion Management. *Transfusion Medicine and Hemotherapy* 44: 106-13.
13. Hanke A, Roberg K, Monaca E, Sellmann T, Weber C, Rahe-Meyer N, et al. Impact of platelet count on results obtained from multiple electrode platelet aggregometry (Multiplate™). *European journal of medical res* 15: 214.
14. Koltai K, Kesmarky G, Feher G, Tibold A, Toth K (2017) Platelet aggregometry testing: Molecular mechanisms, techniques and clinical implications. *Int J molecular sci* 18: 1803.
15. Valsami S, Kollia M, Mougiov V, Sokou R, Isaakidou E, et al. (2020) Evaluation of PFA-100 closure times in cord blood samples of healthy term and preterm neonates. *Clinical Chemistry and Laboratory Medicine (CCLM)* 58: e113-e6.
16. Favaloro EJ (2017) Clinical utility of closure times using the platelet function analyzer-100/200. *American journal of hematology* 92: 398-404.
17. Ostrowsky J, Foes J, Warchol M, Tsarovsky G, Blay J (2004) Plateletworks™ Platelet Function Test Compared to the Thromboelastograph™ for Prediction of Postoperative Outcomes. *J Extracorporeal Technol* 36: 149-52.
18. Raman S, Silverman NA (2001) Clinical utility of the platelet function analyzer (PFA-100) in cardiothoracic procedures involving extracorporeal circulation. *The Journal of thoracic and cardiovascular surgery* 122: 190-1.
19. Fattorutto M, Pradier O, Schmartz D, Ickx B, Barvais L (2003) Does the platelet function analyser (PFA-100®) predict blood loss after cardiopulmonary bypass? *British journal of anaesthesia* 90: 692-3.
20. Forestier F, Coiffic A, Mouton C, Ekouevi D, Chene G, et al. (2002) Platelet function point-of-care tests in post-bypass cardiac surgery: are they relevant? *British journal of anaesthesia* 89: 715-21.
21. Seyfert UT, Haubelt H, Vogt A, Hellstern P (2007) Variables influencing Multiplate™ whole blood impedance platelet aggregometry and turbidimetric platelet aggregation in healthy individuals. *Platelets* 18: 199-206.
22. Rahe-Meyer N, Winterhalter M, Boden A, Froemke C, Piepenbrock S, et al. (2009) Platelet concentrates transfusion

in cardiac surgery and platelet function assessment by multiple electrode aggregometry. *Acta Anaesthesiologica Scandinavica* 53: 168-75.

23. Mengistu M, Wolf M, Boldt J, Roehm K, Lang J, et al. (2008) Evaluation of a New Platelet Function Analyzer in Cardiac Surgery: A Comparison of Modified Thromboelastography and Whole-Blood Aggregometry (Retraction of vol 22, pg 40, 2008). *J Cardiothoracic Vascular Anesthesia* 25: 756-60.

Submit your manuscript to a JScholar journal and benefit from:

- ¶ Convenient online submission
- ¶ Rigorous peer review
- ¶ Immediate publication on acceptance
- ¶ Open access: articles freely available online
- ¶ High visibility within the field
- ¶ Better discount for your subsequent articles

Submit your manuscript at
<http://www.jscholaronline.org/submit-manuscript.php>